



Intelligent Respiratory  
Care Solution

# OmniOx

From Infant to Adult *HFT 700*

A man with brown hair, wearing a blue and white striped button-down shirt, is sitting up in a hospital bed. He is looking out of a window to his right. The room has light-colored wooden furniture and a white cabinet. The overall atmosphere is calm and clinical.

# OmniOx

**MEKICS** strives to have a good understanding of the diseases to be treated and the usage environment of hospitals, and based on clinical issues, endeavors to develop new features and products with the potential to improve such issues and to create a better treatment environment.

**OmniOx** units built with blower, heated humidifier, and built-in oxygen blender was developed as the world's first equipment that integrates heated humidified high oxygen nasal flow cannula treatment with non-invasive positive-pressure ventilation mode as CPAP and bi-level, enabling safe ventilation treatment in various environments from hospital to home.



## Together with from the beginning and to the end of respiratory care

**Omni : Every, All**  
**Ox : Oxygen**

OmniOx is a compound word of the Latin prefix "Omni" meaning "All" or "Every" and the abbreviation "Ox" for oxygen and has various meanings. OmniOx is our original integrated technology for oxygen treatment transcends the limitations of traditional respiratory treatment to provide tailored ventilation treatment from initial respiratory care to weaning, suited to every person and space in need. Our beginning and end aim is for satisfactory results are intended for all patients suffering from respiratory diseases and healthcare professionals who care for the growing number of patients requiring respiratory treatment.

# OmniOx HFT700

## Leading a solution

The OmniOx HFT700 utilizes HF, CPAP and bi-level modes and includes a flow generator, humidifier, built-in oxygen blender, and supports pulse oximeter and connectivity (HL7, WiFi, Bluetooth) as options. In addition, the definition of the product as a “multifunctional non-invasive ventilation treatment device” shows that it is the best product for the environment of non-invasive ventilation treatment.



# Compact

## Supports 3 in 1 device HF, CPAP, and bi-level modes

To meet a variety of requirements of respiratory treatment, it supports a wide range of respiratory treatments, ranging from heated humidified high flow nasal cannula (HFNC) to non-invasive positive-pressure ventilation (NIV). Easy patient installation with medical team management methods give you the flexibility to respond to sudden changes in the patient's symptoms, allowing you to provide efficiently support the patient's respiratory treatment from HF to CPAP or bi-level depending on patient therapy needs within time.

## Built-in blower & oxygen blender

It has a built-in blower that allows you to proactively respond to the medical environment, enabling you to reliably support the patient's respiratory treatment anytime, anywhere. It also allows the built-in oxygen blender to independently control oxygen concentrations from 21% to 100% to provide stable oxygen to the patient.

# Comfort

Improve patient's comfort and safety

## HFNC

Heated humidified high-flow nasal cannula (HFNC) is a patient-friendly and effective treatment for hypoxia because it uses a lighter and more comfortable interface than non-invasive positive pressure ventilation (NIV). It also detects if the circuit is isolated or the cannulas clogged during treatment and sounds an alarm.


## NIV

OmniOx's non-invasive positive pressure ventilation treatment compensates for leaks of up to 60 LPM and uses any type of mask.

# Easy Care

Focus on easy operation for clinician

Real-time monitoring of settings and measurements essential for respiratory treatment is possible, to rapidly respond to sudden changes in the patient's symptoms (FiO<sub>2</sub>, Flow rate, RR, Airway temp, SpO<sub>2</sub>, PR, and S/F ratio). In addition, it is possible to check the history of changes in the patient's symptoms, enabling more efficient treatment.

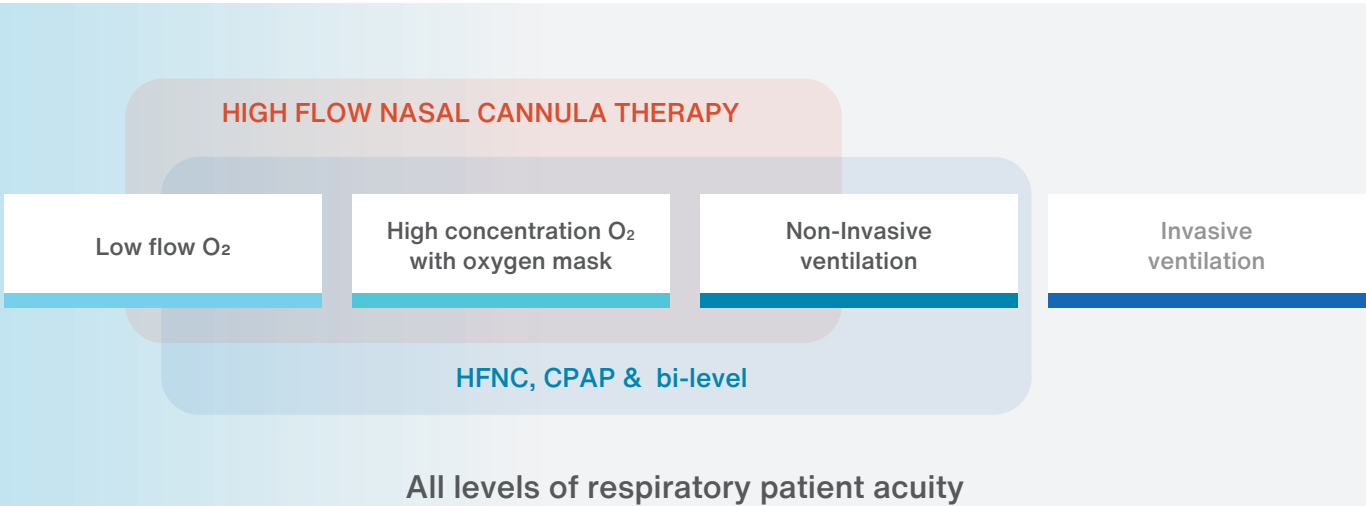



# Fully equipped NIV devices

## Multi-functional non-invasive respiratory care device

### Heated and humidified oxygen administration (Up to 44mg/L)

It enhances pulmonary compliance and conductance compared to traditional cold and dry oxygen-supplied treatments, reducing metabolic work by reducing the gas conditioning process. It also has the advantage of reducing the associated oxygen consumption and carbon dioxide emissions.

### Cannula resistance compensation

It is designed to deliver a set flow rate to the patient by sensing increased resistance, even if the prongs are pressed or bent during heating and humidification high flow nasal cannula therapy. However, if the degree of pressed or bent is in a state where the set flow rate cannot be delivered, an alarm is generated to enable safer breathing treatment.

### Required monitoring features


It monitors the numerical values essential for respiratory treatment to respond quickly to sudden changes in the patient's symptoms. It can monitor FiO<sub>2</sub>, Flow rate, RR, Airway temp, SpO<sub>2</sub>, PR, and S/F ratio, allowing treatment information to be obtained in real time, and makes it possible to check the patient's history, enabling efficient treatment.

## Visible graphic wave

During NIV treatment, numeric values are shown along with flow and pressure figures through graphs, allowing for real-time checking of treatment information.

Monitoring of  $\text{FiO}_2$ , PIP (IPAP), PEEP (EPAP),  $\text{Vt}$  est (estimated tidal volume), RR,  $\text{SpO}_2$ , and PR is supported.

Turn volume guarantee ON to monitor  $\text{FiO}_2$ , V delivery ( $\text{Vi}$ ), PEEP (EPAP), PIP (IPAP), RR,  $\text{SpO}_2$ , and PR.

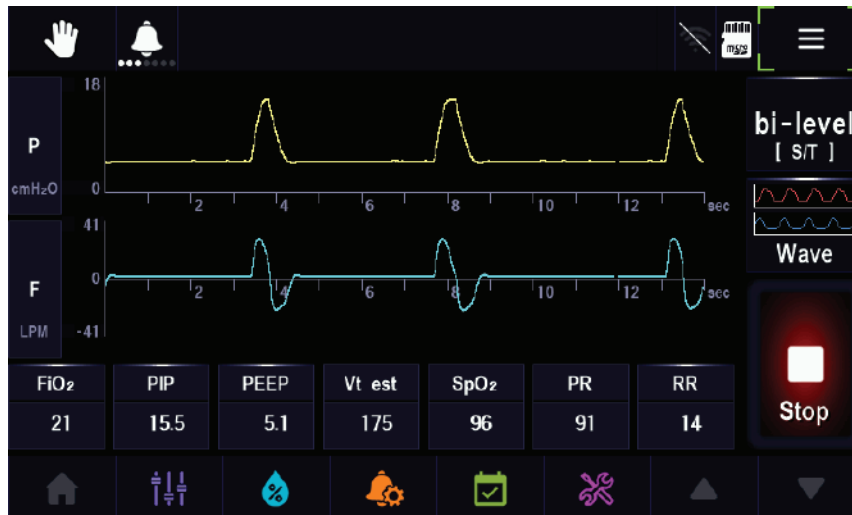


\*Volume guarantee? This function is to convert the target from pressure to volume during inspiration. It can be applied in spontaneous(S), spontaneous / timed(S/T), timed(T) modes, and replaces the inspiration target set value with the tidal volume from the inspiratory positive airway pressure. The provision of tidal volume is limited only by the pressure limit set. Set range: Off, On

## Leak compensation


NIV compensates for leaks of up to 60 LPM, eliminating unnecessary discomfort for the patient and maximizing treatment efficiency. Auto-trigger is enabled in case of an unexpected leak in the interface, or positive end-expiratory pressure (PEEP) is compensated if it is not maintained. It also reliably adjusts and modifies patient trigger sensitivity, minimizing asynchrony.

## Rise time

The time to reach the intake pressure set to rise time is configurable. The shorter the setting time, the higher the peak inspiratory flow rate. In other words, it allows configuration of an intake flow suitable for the patient's inspiratory effort (demand flow).

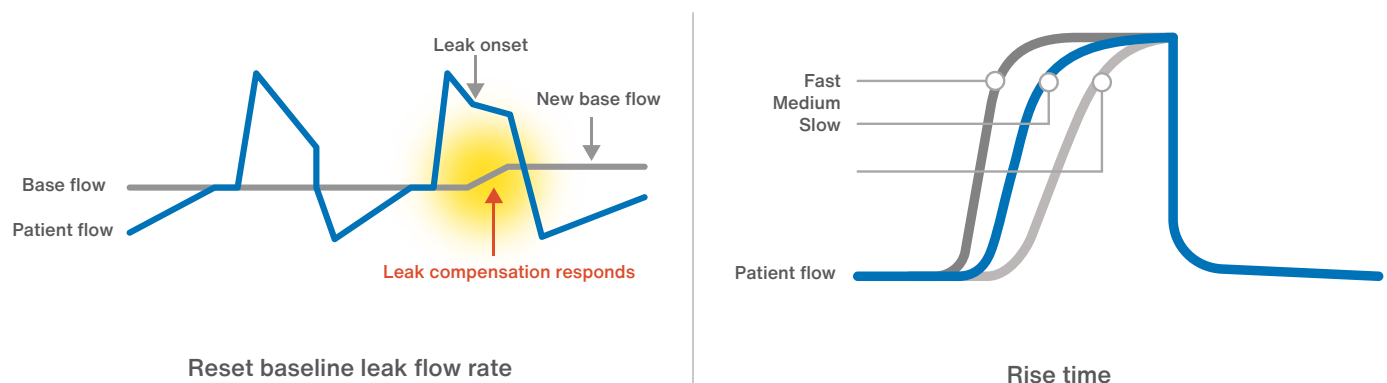

# Easy to use, Simple to set up

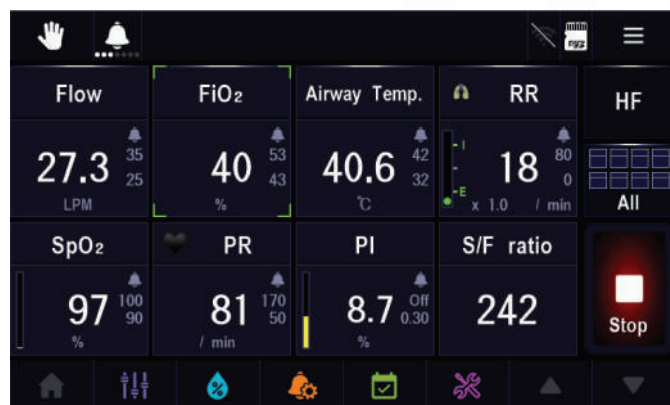

| Parameters  | Mode     |
|---|----------|
| SpO <sub>2</sub> , Airway Temp. ,<br>RR, PR, PI, S/F ratio                                    | HF       |
| SpO <sub>2</sub> , RR, PR, PI, Vt est   | CPAP     |
| SpO <sub>2</sub> , RR, PR, PI,<br>Vt est (Volume guarantee off),<br>PIP (Volume guarantee on) | bi-level |

## All monitoring

When “All monitoring view” type is selected, four additional monitoring parameters are displayed at the bottom of the screen.



## Trend submenu

Sets a time scale per page. You can set the time to 15 minutes, 30 minutes, 1 hour, 3 hours, 6 hours, 12 hours, 24 hours, 72 hours.  
\* Regardless of the setting, the total time stored on the device is equal to 72 hours.

The screenshot shows the 'Event' log screen. It has a list of events with columns for No., Date, Type, Item, and Description. The events include system mode changes, microSD insertions, open circuit alarms, therapy language changes, PEEP high settings, and PIP high alarms. A summary at the bottom indicates 1 / 300 events, with a total of 3000 stored.

| CPAP                            | No.  | Date             | Type    | Item         | Description             |
|---------------------------------|------|------------------|---------|--------------|-------------------------|
| Event                           | 0001 | 21-06-08 [14:17] | System  | Mode         | CPAP                    |
|                                 | 0002 | 21-06-08 [14:17] | System  | microSD      | Inserted                |
|                                 | 0003 | 21-06-08 [14:17] | Alarm   | Open Circuit | Alarm cleared           |
| All                             | 0004 | 21-06-08 [14:17] | System  | Therapy      | Stop                    |
|                                 | 0005 | 21-06-08 [14:17] | System  | Language     | English                 |
| Alarm                           | 0006 | 21-06-08 [14:17] | Alarm   | Open Circuit |                         |
|                                 | 0007 | 21-06-08 [14:17] | Setting | PEEP High    | 8 cmH <sub>2</sub> O    |
| Setting                         | 0008 | 21-06-08 [14:16] | Alarm   | PIP High     | Alarm cleared           |
|                                 | 0009 | 21-06-08 [14:16] | Setting | PIP High     | 20 cmH <sub>2</sub> O   |
| System                          | 0010 | 21-06-08 [14:16] | Alarm   | PIP High     | 10.4 cmH <sub>2</sub> O |
| 1 / 300 [ Total number : 3000 ] |      |                  |         |              |                         |

## Event

Eight events related to alarms, settings, and systems are displayed on the screen. A list displays eight events on one screen. When the event display screen window is activated by touching the screen, pressing the and buttons or rotating the encoder can check eight previous events or eight next events. Events are stored up to a total of 3,000 events. If an event is exceeded, events are deleted in order of occurrence.

# Go beyond limit

## Smart O<sub>2</sub><sup>®</sup> (Target SpO<sub>2</sub> feedback controlled by FiO<sub>2</sub>)


Higher than target SpO<sub>2</sub> : 'Feedback Control' **automatically** support to decrease FiO<sub>2</sub>



Lower than target SpO<sub>2</sub> : 'Feedback Control' **automatically** support to increase FiO<sub>2</sub>



Description of Smart O<sub>2</sub>

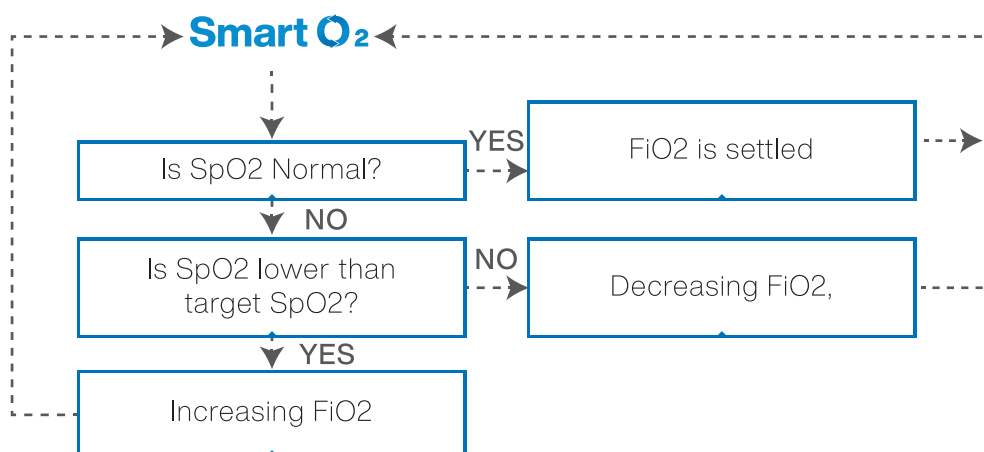


CMS



# For safe use

## Safeguards to minimize infection

The air flowing in from the outside is filtered through the intake filter, and the patient inhales the filtered air through the bacterial filter. Such air intake method minimizes infections. Also, air humidified in the chamber is directly transferred to the interface for patients, which has the advantage of being safe as humidified air does not re-enter the device.

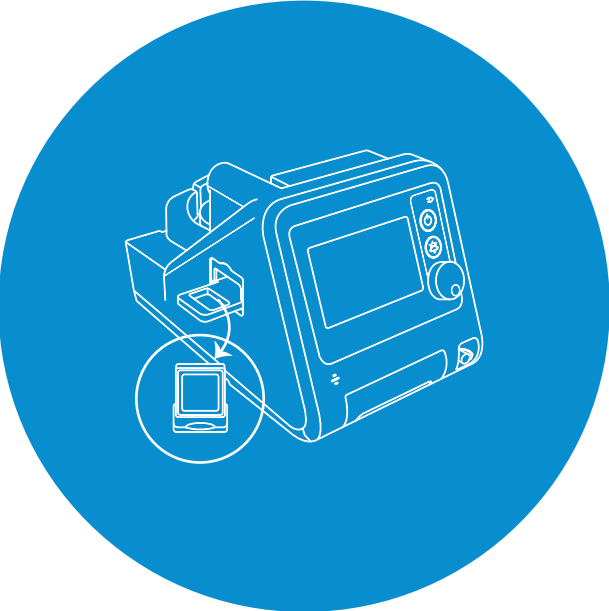


### Air intake filter

| Test article number | Total CFU recovered | Filtration efficiency (%) |
|---------------------|---------------------|---------------------------|
| 1                   | $9.8 \times 10^1$   | 99.9972                   |
| 2                   | $3.6 \times 10^1$   | 99.9990                   |
| 3                   | $5.3 \times 10^1$   | 99.9985                   |

| Test article number | Total CFU recovered | Filtration efficiency (%) |
|---------------------|---------------------|---------------------------|
| 1                   | $1.5 \times 10^3$   | 99.982                    |
| 2                   | $1.3 \times 10^3$   | 99.985                    |
| 3                   | $2.1 \times 10^3$   | 99.975                    |

\* Test results from Nelson Laboratories, Inc. (NLI)

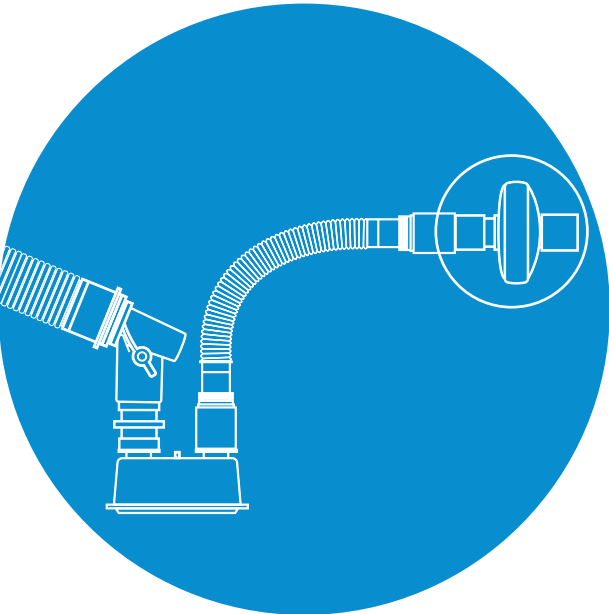

### Bacterial filter

| Test article number | Total CFU recovered | Filtration efficiency (%) |
|---------------------|---------------------|---------------------------|
| 1                   | $3.1 \times 10^1$   | 99.99983                  |
| 2                   | $1.0 \times 10^1$   | 99.99946                  |
| 3                   | $2.6 \times 10^1$   | 99.99986                  |
| 4                   | $2.6 \times 10^1$   | 99.99986                  |
| 5                   | $2.1 \times 10^1$   | 99.99989                  |

| Test article number | Total CFU recovered | Filtration efficiency (%) |
|---------------------|---------------------|---------------------------|
| 1                   | $8.6 \times 10^2$   | 99.9952                   |
| 2                   | $8.6 \times 10^2$   | 99.9952                   |
| 3                   | $1.4 \times 10^3$   | 99.9923                   |
| 4                   | $5.3 \times 10^2$   | 99.9970                   |
| 5                   | $1.0 \times 10^3$   | 99.9943                   |

\* Test results from Nelson Laboratories, Inc. (NLI)

# Specificaion

## HF (High Flow)

---

|                              |  |
|------------------------------|--|
| Flow (Inspiratory flow rate) | 1 ~ 60 LPM   |
| RR Sensitivity               | x0.2 ~ x3.0  |
| RR detection                 | OFF<br>Internal sensor<br>Respiratory detection Line (With an external RR detection accessory) |

## CPAP (Continuous Positive Airway Pressure)

---

|                           |   |
|---------------------------|---|
| CPAP                      | 4 ~ 20 cmH2O $\pm(1.7 + 4 \%$ of the set value) cmH2O |
| Pressure Assist + (PA(+)) | OFF, 1 ~ 3 cmH2O                                      |
| Pressure Assist - (PA(-)) | OFF, -3 ~ -1 cmH2O                                    |
| Trigger Level             | 3 ~ 20 lpm  |
| Rise time                 | Fast(0.2 sec), Medium(0.3 sec), Slow(0.4 sec)         |
| Auto Start                | ON, OFF   |

## bi-level Positive Airway Pressure (Spontaneous, Spontaneous / Timed, Timed )

---

|                           |   |
|---------------------------|---|
| IPAP                      | 4 ~ 40 cmH2O $\pm(1.7 + 4 \%$ of the set value) cmH2O |
| EPAP                      | 4 ~ 20 cmH2O $\pm(1.7 + 4 \%$ of the set value) cmH2O |
| Pressure Assist - (PA(-)) | OFF, -3 ~ -1 cmH2O                                    |
| Respiration Rate          | 2 ~ 60 bpm  |
| Inspiratory Time(Ti)      | 0.3 ~ 3.0 seconds                                     |
| Trigger Level             | 3 ~ 20 lpm  |
| Trigger Type              | S/T, T, S   |
| Rise time                 | Fast(0.2 sec), Medium(0.3 sec), Slow(0.4 sec)         |
| Auto Start                | ON, OFF   |

## Common

---

|        |               |  |
|--------|---------------|--|
| FiO2 % | High pressure | 21, 25 ~ 100 %, Electronic controlled blender (built-in system)<br>Accuracy : $\pm 5 \%$ |
|        | Low flow      | Device does not support oxygen concentration control.<br>(Only FiO2 monitoring)          |

- Pulse oximeter can be provided with the two options: MEK, Masimo



**MEKICS. CO., Ltd**

**Headquarter / Factory**

21, Sangjiseok-gil, Paju-si, Gyeonggi-do, South Korea 10911

**Branch Office**

12, Moraenae-ro 7-gil, Mapo-gu, Seoul, South Korea 03949

[www.mek-ics.com](http://www.mek-ics.com)